

216.681

170.507

79.932
78.435
77.478
77.161
76.843
66.378
60.458
52.033
49.324
49.252
46.224
45.861
38.735
38.385
37.765
34.630
34.428
31.474
28.242
27.641
26.936
24.342
20.608
18.925
18.796
15.535
13.493
13.450
0.141



Current Data Parameters
NAME GG
EXPNO 2
PROCNO 1


F2 - Acquisition Parameters
Date_ 20140504
Time 20.41
INSTRUM spect
PROBHD 5 mm PABBO BB-
PULPROG zgpg30
TD 65536
SOLVENT CDC13
NS 2500
DS 4
SWH 24038.461 Hz
FIDRES 0.366798 Hz
AQ 1.3631988 sec
RG 194.85
DW 20.800 usec
DE 6.50 usec
TE 300.5 K
D1 2.00000000 sec
D11 0.03000000 sec
TD0 1

===== CHANNEL f1 =====
NUC1 13C
P1 9.24 usec
PLW1 95.00000000 W
SF01 100.6228293 MHz

===== CHANNEL f2 =====
CPDPRG2 waltz16
NUC2 1H
PCPD2 80.00 usec
PLW2 19.00000000 W
PLW12 0.25292000 W
PLW13 0.16187000 W
SF02 400.1316005 MHz

F2 - Processing parameters
SI 32768
SF 100.6127533 MHz
WDW EM
SSB 0
LB 1.00 Hz
GB 0
PC 1.00

200 180 160 140 120 100 80 60 40 20 ppm

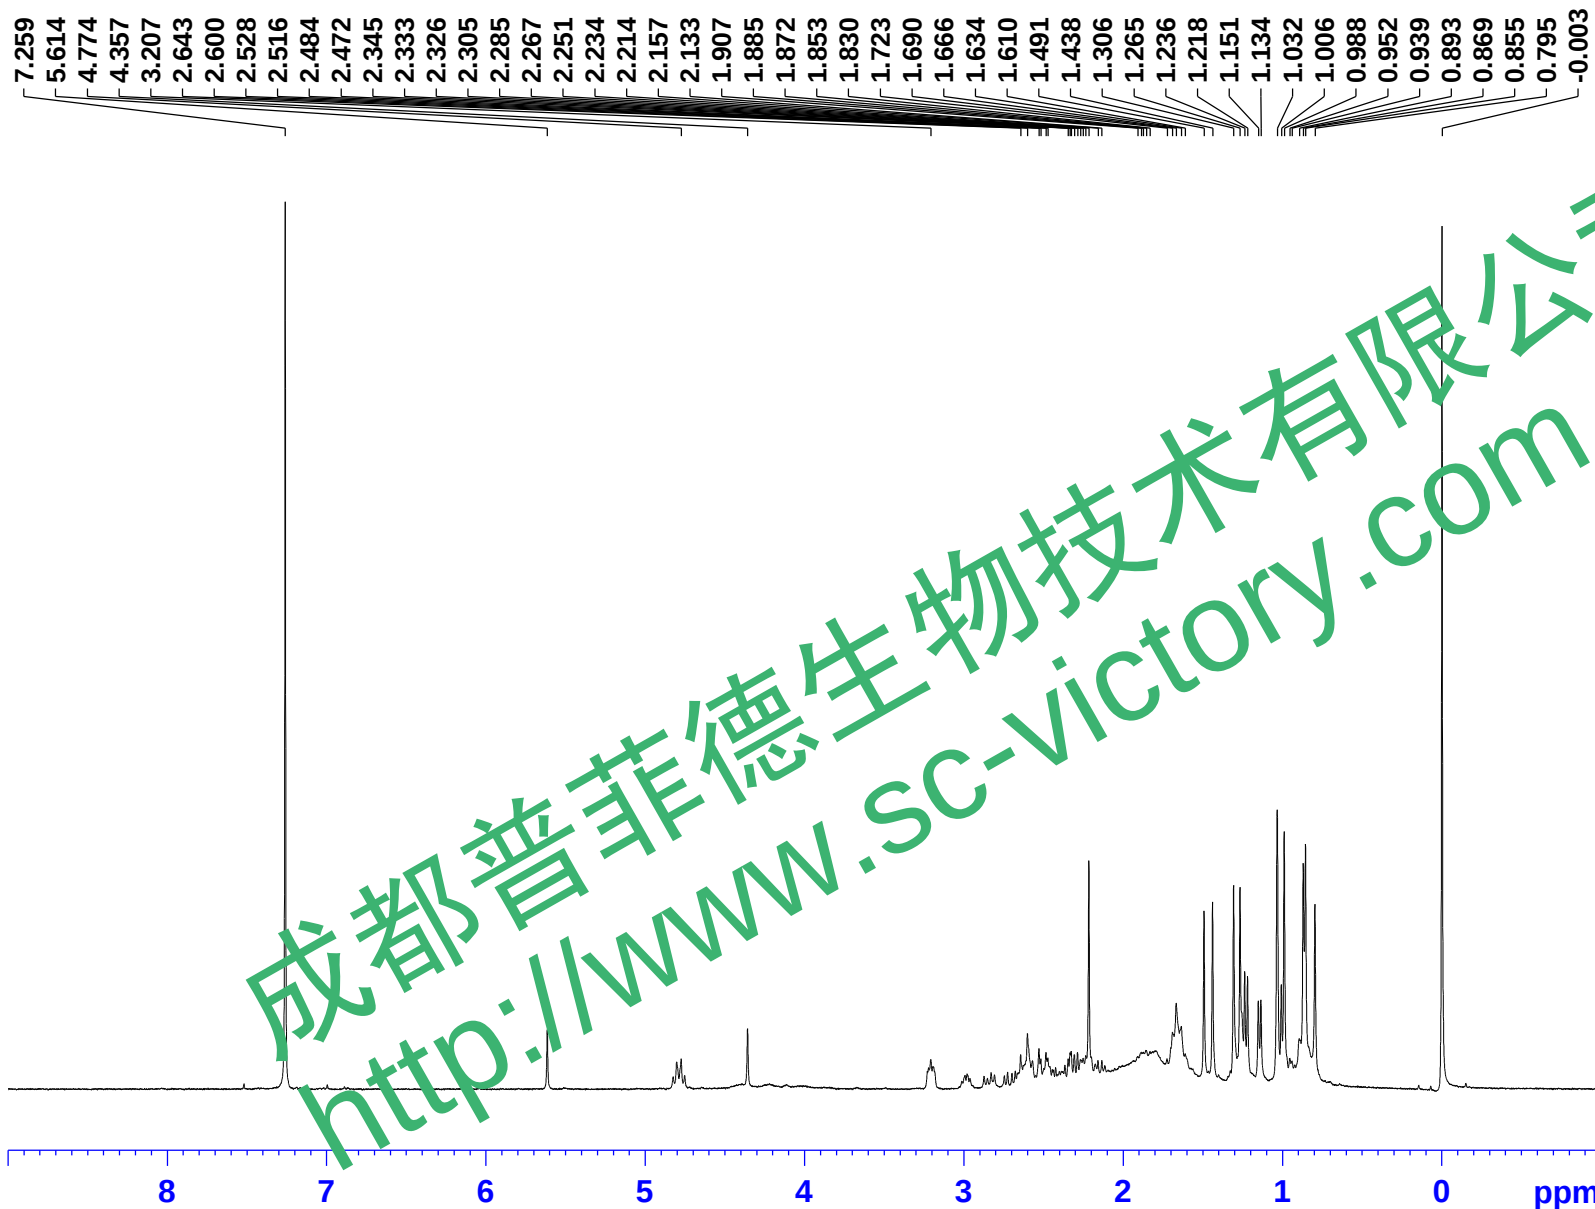

Current Data Parameters
NAME GG
EXPNO 1
PROCNO 1

F2 - Acquisition Parameters
Date_ 20140504
Time 18.17
INSTRUM spect
PROBHD 5 mm PABBO BB-
PULPROG zg30
TD 65536
SOLVENT CDC13
NS 16
DS 2
SWH 8223.685 Hz
FIDRES 0.125483 Hz
AQ 3.9846387 sec
RG 124.98
DW 60.800 usec
DE 6.50 usec
TE 299.6 K
D1 1.00000000 sec
TD0 1

===== CHANNEL f1 =====
NUC1 1H
P1 9.23 usec
PLW1 20.00000000 W
SF01 400.1324710 MHz

F2 - Processing parameters
SI 65536
SF 400.1300101 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00